

The  
**Sleep Technician's  
Pocket Guide**

**A Quick Reference Manual**

**WILLIAM H. SPRIGGS, BS, RPSGT**



**JONES AND BARTLETT PUBLISHERS**

*Sudbury, Massachusetts*

**BOSTON    TORONTO    LONDON    SINGAPORE**

## **World Headquarters**

Jones and Bartlett Publishers  
40 Tall Pine Drive  
Sudbury, MA 01776  
978-443-5000  
info@jbpub.com  
www.jbpub.com

Jones and Bartlett Publishers  
Canada  
6339 Ormindale Way  
Mississauga, Ontario L5V 1J2  
Canada

Jones and Bartlett Publishers  
International  
Barb House, Barb Mews  
London W6 7PA  
United Kingdom

Jones and Bartlett's books and products are available through most bookstores and online booksellers. To contact Jones and Bartlett Publishers directly, call 800-832-0034, fax 978-443-8000, or visit our website, [www.jbpub.com](http://www.jbpub.com).

Substantial discounts on bulk quantities of Jones and Bartlett's publications are available to corporations, professional associations, and other qualified organizations. For details and specific discount information, contact the special sales department at Jones and Bartlett via the above contact information or send an email to [specialsales@jbpub.com](mailto:specialsales@jbpub.com).

Copyright © 2010 by Jones and Bartlett Publishers, LLC

All rights reserved. No part of the material protected by this copyright may be reproduced or utilized in any form, electronic or mechanical, including photocopying, recording, or by any information storage and retrieval system, without written permission from the copyright owner.

The author and publisher have made every effort to provide accurate information. However, they are not responsible for errors, omissions, or for any outcomes related to the use of the contents of this guide. The user is advised to carefully consult their medical director prior to making any deviations from locally accepted protocols and guidelines.

Printing and Binding: Imago

Cover Printing: Imago

ISBN: 978-0-615-26154-6

6048

Printed in Hong Kong

13 12 11 10 09 10 9 8 7 6 5 4 3 2 1

© Jones and Bartlett Publishers, LLC. NOT FOR SALE OR DISTRIBUTION.

## -Table of Contents-

---

<b>Section 1: Patient Hookup</b>	<b>2</b>
International 10/20 System	3-10
Face Electrodes	11-16
Body Electrodes	17-23
EEG Measurement Guide	24
<b>Section 2: Artifacts/Troubleshooting</b>	<b>25</b>
Signal Pathways	26
Artifacts	27-35
Correcting Artifacts	36-37
<b>Section 3: Scoring</b>	<b>38</b>
Sleep Staging	39-48
Sleep Events	49-66
Formulas, & Calculations	67-69
Norms and Averages	70-72
Arterial Blood Gas Values	73
<b>Section 4: EKG Rhythms</b>	<b>74</b>
Reading EKG's	75

Sinus Rhythms	76-79
Atrial Rhythms	80-82
Ventricular Rhythms	83-87
AV Blocks	88-91

<b>Section 5: Procedures &amp; Protocol</b>	<b>92</b>
Order of Operations	93
Items for the Patient Tray	94
Physiologic Calibrations	95
Technician Notes	96
Sample Montages	97-101
Sample Protocols	102-105
MSLT Procedures	106
Body Mass Index Tables	107-108

<b>Section 6: Drugs &amp; Medications</b>	<b>109-117</b>
---	----------------

<b>Section 7: Glossary</b>	<b>118-156</b>
----------------------------	----------------

---

## Patient Hookup


This section contains step-by-step information regarding patient hookup procedures. While electrode application processes may vary among

technicians, proper placement on the head and body remains a key to performing a quality sleep study.

## International 10/20 System

The following EEG electrode sites are used in a standard overnight sleep study:


- F3
- F4
- C3
- C4
- O1
- O2
- M1
- M2
- FpZ

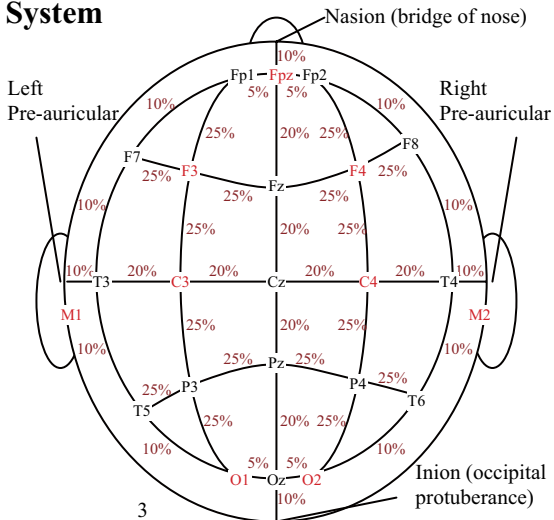

# International 10/20 System

## Step 1: Locate the 4 Landmarks


- The **nasion** is the bridge of the nose
- The **inion** is the most prominent point of the occipital bone
- The **pre-auricular points** are just in front of the notches in the middle of each ear

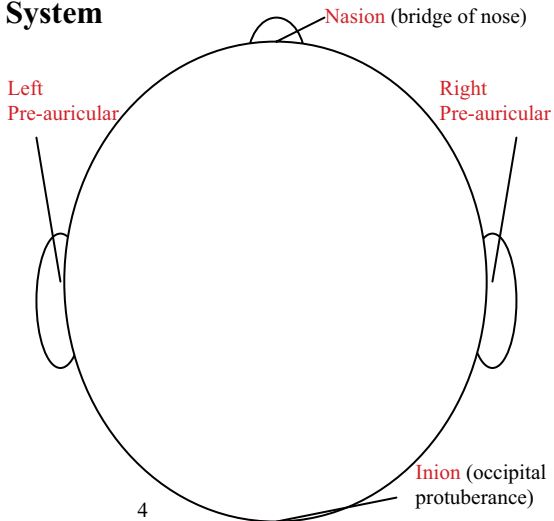

## International 10/20 System

### Step 2: Measure and Mark Between the Nasion and Inion

Measure the distance between the nasion and inion, across the top of the head. Mark 10% of the total distance in the front and back. Mark the halfway point (50%). Mark 20% down from the halfway point in the front.

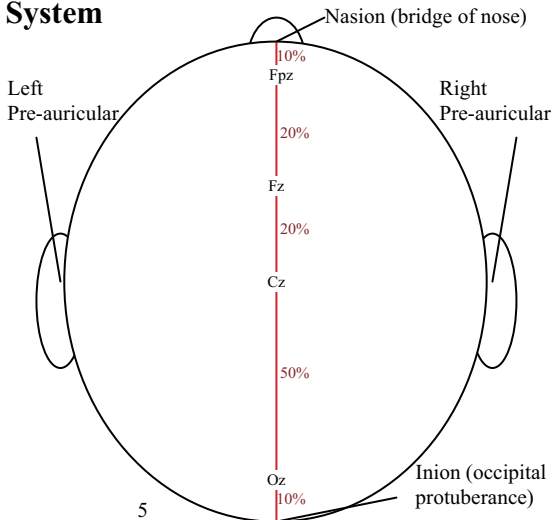

## International 10/20 System

### Step 3: Measure and Mark Between the Pre-Auricular Points

Measure the distance between pre-auricular points with the tape through the 50% mark from step 1. Mark 10% up on each side. Mark the 50% point. Mark 20% down from the halfway point on the right and left sides.

